MITEL 5000 Communications Platform (CP) System Administration & Diagnostics

Guide





Mitel System Administration & Diagnostics Guide

Issue 5.0, February 2011

Notice

This manual is released by Mitel Networks Corporation as a guide for certified service personnel. It provides information necessary to properly configure, maintain, and operate the product.

The contents of this document reflect current company standards and are subject to revision or change without notice. Some features or applications mentioned may require a future release and are not available in this release. Future product features are subject to availability and cost. Some features may require additional hardware and/or specific software.

The contents of this manual may include technical or other inaccuracies. Mitel reserves the right to make revisions or changes without prior notice. Software packages released after the publication of this manual will be documented in addenda to the manual or succeeding issues of the manual.

For additional information and/or technical assistance in North America, certified technicians may contact:

Mitel Networks Corporation Technical Support Department (USA) 7300 West Boston Street Chandler, AZ 85226-3224 1-888-777-EASY (3279)

For information on how to contact Mitel Technical Support outside of North America, please refer to your Channel Support Agreement.

If you have any questions or comments regarding this manual or other technical documentation, contact the Technical Publications Department (USA) at:

tech_pubs@mitel.com

Mitel[®] is a registered trademark of Mitel Networks Corporation.

All other trademarks mentioned in this document are the property of their respective owners, including Mitel Networks Corporation. All rights reserved.

© 2010-2011 Mitel Networks Corporation

Personal use of this material is permitted. However, permission to reprint/republish this material for advertising or promotional purposes or for creating new collective works for resale or redistribution to servers or lists, or to reuse any copyrighted component of this work in other works must be obtained from Mitel Networks Corporation.

Limited Warranty

Mitel warrants that its products will, if delivered to the end-user in undamaged condition, be free from defects in material and workmanship under normal use and service for the period set forth on the current warranty periods as published in the U.S. Price List from time to time and substantially in conformance with the documentation (functional and operating specifications) that Mitel publishes regarding same (end-user reference and operating manuals and guides relating to the program). Mitel does not, however, warrant that the functions contained in the software program will satisfy Dealer's particular purpose and/or requirements or that the operation of the program will be uninterrupted or error free.

Mitel shall incur no liability under this warranty and this warranty is voidable by Mitel (a) if the product is used other than under normal use, with certified repair and maintenance service and under proper environmental conditions, (b) if the product is subject to abuse, misuse, neglect, flooding, lightning, power surges, third-party error or omission, acts of God, damage, or accident, (c) if the product is modified or altered (unless expressly authorized in writing by Mitel), (d) if the product is installed or used in combination or in assembly with products not supplied or authorized by Mitel and/or which are not compatible with or are of inferior quality, design, or performance to Mitel or Mitel supplied products so as to cause a diminution or degradation in functionality, (e) if there is a failure to follow specific restrictions in operating instructions or (f) if payment for product has not been timely made.

The sole obligation of Mitel and the exclusive remedy and recourse of Dealer under this warranty, or any other legal obligation, with respect to product, including hardware, firmware, and software media, is for Mitel, at its election, to either repair and/or replace the allegedly defective or missing product(s) or component(s) and return (prepaid) same (if necessary), or grant a reimbursement credit with respect to the product or component in the amount of the sales price to the Dealer. With regard to a software program design defect, however, to the extent it prevents the program from providing functionality and/or operating as intended by Mitel, is service affecting, and prevents beneficial use of the product, Mitel does undertake to use its best efforts to devise a suitable corrective solution to the problem within a reasonable period of time; should said action, however, not substantially resolve the problem, then Mitel reserves the right to substitute a new release ("stream") of software as soon as it is generally made available by Mitel. The above, with regard to a software design defect, likewise, constitutes the sole obligation of Mitel and exclusive remedy of Dealer hereunder.

The responsibility of Mitel to honor the express limited warranty stated above also shall be predicated on receiving timely written notice of the alleged defect(s) with as much specificity as is known within thirty (30) calendar days of the malfunction or by the expiration of the warranty period (plus thirty [30] calendar days), whichever occurs first. Mitel shall further have the right to inspect and test the product to determine, in its reasonable discretion, if the alleged malfunction is actually due to defects in material or workmanship. Unless waived by Mitel, Dealer agrees to return (prepaid) the allegedly defective product or component to Mitel for inspection and/or testing, and, if appropriate, for repair and/or replacement.

NOTICE

The above express Limited Warranty is in lieu of all other warranties, express or implied, from Mitel Networks Corporation, or Inter-Tel, Inc., and there are no other warranties which extend beyond the face of this warranty. All other warranties whatsoever, including the implied warranty of merchantability and the implied warranty of fitness for a particular purpose relating to use or performance of the product, including its parts, are hereby excluded and disclaimed.

In no event shall Mitel Networks Corporation, under any circumstances, be liable for nor shall a purchaser (directly or indirectly) be entitled to any special, consequential, incidental, indirect, punitive, or exemplary damages as a result of the sale or lease of product including but not limited to failure to timely deliver the product or failure of product to achieve certain functionality, or arising out of the use or inability to use the product, in whole or in part and including but not limited to loss of profit, loss of use, damage to business or damage to business relations even if notified of the possibility of such damages. Mitel shall not be liable for personal injury or property damage unless caused solely by Mitel's negligence.

Network Security Statement

Although no telecommunications system or data network is entirely secure, as long as appropriate security measures are put in place and properly maintained by both the customer and the installing company, this Mitel[®] Communications Platform architecture and its associated server-based applications are substantially secure against unauthorized access to the customer's data network via the telecommunications system. Appropriate security measures include, but are not limited to, the proper implementation of user/administrative accounts, passwords, firewalls, Network Address Translation (NAT), access control lists, virus protection, security updates, etc., and the proper maintenance of access points/programs and their respective accounts/passwords.

Contents

Overview	1
Introduction	2
About this Guide	
User Types	4
Connection Types	4
Compatibility	5
Specifications	6
Hardware Requirements	6
Software Requirements	6
Network Requirements	6
Licensing	6
Understanding the Interface	7
Introduction	
Navigation	9
Title Bar	9
Information Bar	9
Navigation Area	10
Content Controls	12
System Connection Section	15
System Monitoring Section	17
Menu Buttons	18
Tooltips	19
Warning Message Boxes	19
Installing and Launching the Application	21
Introduction	22
Installing the Application	22
Launching the Application	24
Importing Connections	25
Adding Connections Manually	25
Exiting without Adding or Importing Connections	28
Enabling an On-Demand Remote Connection from a phone	29
Upgrading from Older Software	30
Programming the Application	31
Index	33

Overview

Introduction	2
About this Guide	3
User Types	4
Connection Types	4
System Connections	4
DB Programming Connections	5
Compatibility	5
Specifications	6
Hardware Requirements	3
Software Requirements	3
Network Requirements	3
Licensing	6

Introduction

System Administration & Diagnostics is a new personal computer (PC)-based application that provides a single interface to access all of the administration and system monitoring tools available on the Mitel 5000 Communications Platform (CP). Using this application, you can easily configure and upgrade the system, monitor active calls, view resource usage, troubleshoot issues, and so forth.

Mitel 5000 CP Database (DB) Programming is installed as part of the System Administration & Diagnostics application along with other supporting system management tools and utilities. After installing the System Administration & Diagnostics application, you can launch any of the following:

- DB Programming
- Administrative Web Session (AWS)
- Secure Shell (SSH) Connection (PuTTY)
- Database Converter
- MOH (Music-on-Hold) Converter
- Test and Repair
- Upload Utility

After establishing a connection to a 5000 CP node, System Administration & Diagnostics queries call, resource/device, system, and system status data from the node. It then uses a variety of content controls to display this information in a well-organized manner that allows you to easily read and understand the data. The application automatically receives updates periodically, but also allows you to refresh data on demand.

NOTE

The system monitoring portion of System Administration & Diagnostics can be very useful for occasional monitoring of system usage and troubleshooting. As with any tool that monitors system activity, this monitoring may have a slight impact on system performance. The impact is directly related to the size of the system (number of devices), as well as the number of concurrent active System Administration & Diagnostics sessions connected to the system. If there is a noticeable difference in system performance after upgrading to v4.0 or later and/or when multiple System Administration & Diagnostics sessions are connected to a system, contact Technical Support.

Throughout the following chapters of this manual, change (revision) bars like the one next to this paragraph have been placed in the margins to indicate significant changes or additions since the previous publication of this manual (Issue 1.0, June 2010).

About this Guide

This Mitel System Administration & Diagnostics Guide includes the following chapters:

- Overview: Provides an overview of the System Administration & Diagnostics application and defines hardware, software, and network specifications.
- Understanding the Interface: Summarizes the functionality of the user interface (UI), such as bars, menu buttons, sections, and content controls, in the System Administration & Diagnostics window.
- Installing and Launching the Application: Provides instructions for installing and launching the application. This chapter also provides considerations when upgrading from older software.

For programming instructions, refer to the Mitel System Administration & Diagnostics Help.

To access the online help:

Press **F1** or the Help menu button () in the upper-right corner of the application interface.

The Help contains the following information:

- About System Administration & Diagnostics: Provides information about an overview of the System Administration & Diagnostics application. This is the same information described in the Overview chapter in this guide.
- Understanding the Interface: Summarizes the functionality of the System Administration & Diagnostics UI. This is the same information described in the Understanding the Interface chapter in this guide.
- Getting Started: Provides instructions for launching the application and information for upgrading. This section also provides the instructions for programming scheduled backups.
- **Managing System Connections**: Provides information for programming, managing, and using system connections, DB Programming, and management tools.
- Using System Monitoring Tools: Provides information for programming, managing, and using system monitoring content controls and tools.
- **Using the Menu Buttons**: Provides information for programming, managing, and using the Utilities, Setup, and Help menu buttons.
- Diagnostics and Troubleshooting: Provides information that helps you to diagnose and troubleshoot issues that are associated with System Administration and Diagnostics.

User Types

The System Administration & Diagnostics application supports two user types. The System Administration & Diagnostics UI is customized for each user type so only the most appropriate data is presented:

- System Administrator (default): Intended to be used by end users and field technicians.
- Mitel Support: Intended to be used by technical support personnel. Supports all of the features and options for the System Administrator user type and provides additional system monitoring information in the following areas:
 - System Monitoring option
 - o Current Calls information
 - IPDRM Resource Usage information
 - o Application information
 - System Command information
- Reporting User: Intended to be used by "business-level" users who are not system
 administrators. When the Reporting User type is selected, the main UI is simplified to
 show just the Reporting tab. In addition, the System management tools button and the
 System Monitoring section are hidden.

NOTE

The user type does not correlate to the log-in account types in DB Programming. The log-in account is determined based on the System Account settings in DB Programming. The user type is determined based on the settings in System Administration & Diagnostics.

Connection Types

When the System Administration & Diagnostics application is connected to a 5000 CP, that connection is defined as a system connection (or sometimes referred to as a node).

System Connections

Each system connection can have one onsite connection and one offsite connection and supports the following connection types:

- Onsite: Connects to the 5000 CP using an IP connection.
- Offsite: Connects to the 5000 CP using various methods:
 - Modem: Connects to the 5000 CP using an onboard modem.
 - Network: Connects to the 5000 CP using an external (NATed) IP connection.
 - Remote Configuration: (Reserved for controlled introduction.) If authorized, you can
 use the Remote Configuration feature to access the 5000 CP using a Virtual Private
 Network (VPN) connection. Refer to the Mitel 5000 Features and Programming Guide,
 part number 580.8006 for details.

Multiple on-site connections are allowed for running system monitoring. Multiple off-site connections, however, are not allowed due to the contention of the Modem/Remote Configuration connection.

DB Programming Connections

You can use a single instance of the System Administration & Diagnostics application to launch or open multiple DB Programming sessions that can run simultaneously, similar to the capability provided by the Session Manager in pre-v4.0 systems. When a system connection is established, you can launch or open the following DB Programming sessions:

- **Online session**: A session that is connected to the 5000 CP (a.k.a. "remote" session in pre-v4.0 systems).
- Offline session: A stand-alone session that is not connected to the 5000 CP (a.k.a. "local" session in pre-v4.0 systems).

Compatibility

Although System Administration & Diagnostics is introduced as part of the 5000 CP v4.0 or later release, this application can manage the system connections for all previous versions of the 5000 CP. When connected to a pre-v4.0 system, advanced system monitoring capabilities of System Administration & Diagnostics are not available, however, the system connection management, DB Programming connectivity, and utilities/tools are still available.

When system monitoring capabilities are not supported (on pre-v4.0 systems), the content controls appear dimmed and are overlaid with the text "Unavailable." To use as much functionality as possible, refer to the Launching a pre-v4.0 DB Programming help topic in the *Mitel System Administration & Diagnostics Help*. See page 30 for details about upgrading from older software.

Connections to Axxess systems are not supported and are not impacted by the installation of this application.

Specifications

The following section describes the hardware, software, and network requirements for the System Administration & Diagnostics application.

Hardware Requirements

The following lists the hardware requirements for the System Administration & Diagnostics application:

- 1.0 gigahertz (GHz) or higher Central Processing Unit (CPU)
- 1 gigabyte (GB) or higher Random-Access Memory (RAM)
- 1024x768 high-color 32-bit display
- 100 megabytes (MB) available hard disk space (not including the space needed for the .NET Framework)

Software Requirements

The following lists the software requirements for the System Administration & Diagnostics application:

- Microsoft[®] Windows[®] XP (SP2/SP3), Window Vista[®] (SP1), or Windows 7
- Microsoft .NET Framework version 4.0 (included in the installation program)

Network Requirements

The System Administration & Diagnostics application requires a Network (or Modem) connection to connect to the 5000 CP. Each instance of the System Administration & Diagnostics application can gather data for one node.

Licensing

The System Administration & Diagnostics application does not require a license.

Understanding the Interface

Intr	oduction
Nav	vigation
	Title Bar
	Information Bar 9
	Navigation Area
	Content Controls
	System Connection Section
	System Connection
	System Management Tools
	System Monitoring Section
	Buttons
	Alarm Counts
	Menu Buttons
	Tooltips
	Warning Message Boxes


Introduction

The System Administration & Diagnostics UI contains the following sections: Title bar, Information bar, navigation area, content controls, System Connection and System Monitoring sections, menu buttons, and expand/collapse button. Each section is described in the following pages.

The System Administration & Diagnostics UI operates in expanded and collapsed modes. The System Monitoring section contains a button to toggle between expanded and collapsed mode (see 3 below):

Expanded Mode: This is the default mode and displays the full system monitoring capabilities.


Figure 1. System Administration & Diagnostics UI in Expanded Mode

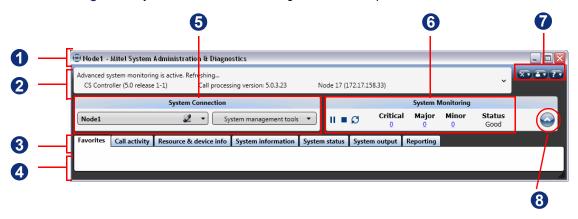

- 1 Title Bar (see page 9) 5 System Connection Section (see page 15)
- 2 Information Bar (see page 9) 6 System Monitoring Section (see page 17)
- 3 Navigation Area (see page 10) 7 Menu Buttons (see page 18)
- 4 Content Controls (see page 12) 8 Expand/Collapse Button (see page 18)

Collapsed Mode: Displays almost all of the system monitoring capabilities, except for the navigation area and content controls. The collapsed mode is used in situations where the system monitoring features are not necessary, are not authorized, or are not available. For example, if you simply want to use DB Programming, you may choose to use the collapsed mode. When you decide to use the system monitoring features, click the Expand/Collapse button to switch to the expanded mode.

Figure 2. System Administration & Diagnostics UI in Collapsed Mode



Navigation

The following pages summarize the functionality of each section in the System Administration & Diagnostics window.

Title Bar

The Title bar displays the official application product name and icons that allow you to minimize, maximize, and exit the application. The Windows taskbar item for the application shows the name of the active connection followed by the application name (for example, "Node 1 - Mitel System Administration & Diagnostics").

Information Bar

Figure 3 shows an example of the Information bar.

Figure 3. Information Bar



The Information bar is made up of the following parts:

- Status Indicator: Appears while connecting to a system.
- System Connection Header: Displays general status information regarding the currently active system connection. This header is always visible. If a message appears indicating that advanced system monitoring is inactive, press ▶ (Start monitoring system) to start data updates manually (see page 17). To start system monitoring automatically, select the Start system monitoring option in the General tab in the Options dialog box. Refer to the System Administration & Diagnostics Help for details.
- Buttons: Appear in the Information bar when connection operations are available.
 Depending on the state of the connection, the available buttons are the Keep waiting, Edit Connection, Retry, Connect, Cancel, Cancel retry, and Disconnect buttons.
- Status Details: Displays additional connection information. As a connection is being
 established, the progress appears. After a connection has been established, the platform
 type, software version, and IP address appear. If a connection fails to be established, the
 details of the failure appear. It is in an expansion area that can be displayed and hidden by
 clicking on the Header text area.
- Expand/Collapse Indicator: Shows the status of the expansion area, pointing down to
 indicate it is collapsed and can be expanded, and pointing up to indicate it is expanded
 and can be collapsed. If there is no detail to be displayed in the expansion area, the
 indicator does not appear and clicking on the bar does nothing.

Navigation Area

The navigation area contains tabs which separate the system monitoring information into different categories. The content of each tab is comprised of a collection of content controls.

Figure 4 shows an example of the navigation tabs.

Figure 4. Navigation Tabs



Each of the navigation tabs consist of multiple content controls. These content controls can be expanded or collapsed. You can drag the content controls around on the tab to arrange and reorder them. The content controls are arranged horizontally on the tab. If a control does not fit on the current row, it wraps to the next row. See page 12 for an example of the content control.

Table 1 shows brief tab descriptions and available content controls for each tab. See appropriate pages for details. For details about tabs and contents, refer to the *Mitel System Administration & Diagnostics Help*.

Table 1. Tabs and Content Controls

Tab	Description	Content Control
Favorites	Customizes the system monitoring view by selecting items that are most important for their needs.	N/A
Call activity	Displays statistics and data related to the calls	Hourly Call Statistics
	on the system.	Current Calls
		Call Traffic
Resource &	Displays information about current resource	Phones
device information	status and usage.	IP Resource Usage
		IPDRM (IP Device Resource Manager) Resource Usage ^a
System	Displays information related to the system	System Information
information	application / package, software license, system upgrade, and node.	Networking Information
		Application Information
System status	Displays information regarding system	System Utilization
	utilization, last system reset, bay/module status, call status, and errors and warnings.	System Alarms
	3 .	Bay/Module Status
System output	Generates various diagnostic reports using	Message Print
	Message Print and diagnostics commands.	System Commands ^a

Table 1. Tabs and Content Controls (Continued)

Tab	Description	Content Control
Reporting	information using charts and data grids.	Call Distribution Report
		PSTN Call Records Report
		Hunt Groups Report
		Voice Mail Report b
		Mailboxes Report ^b
		Configured Devices Report
		Database Reporting ^c

- a. Applicable to Mitel Support users only.
- b. Visible only when Unified Voice Messaging (UVM) is configured on the system.
- c. To support Database Reporting, the SAP® Crystal Reports® application (built with Crystal Reports for Microsoft® Visual Studio® 2010) must be installed during the System Administration & Diagnostics installation. The installation also includes the Microsoft Access® 2010 Runtime redistributable program.


Content Controls

Each navigation tab is made up of a collection of content controls. The content controls provide the diagnostic information in an easy to understand, self-contained format.


Figure 5 shows an example of the IP Resource Usage content control.

Figure 5. Content Control

Expanded Mode

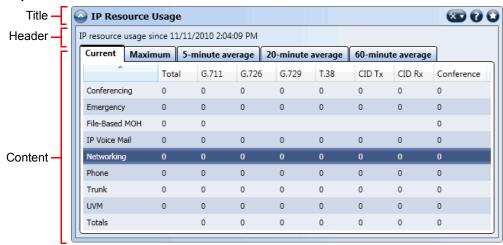

Collapsed Mode

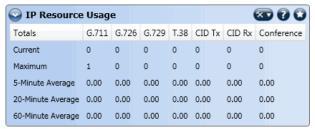

Content controls consist of the following areas:

 Title: Includes an expand/collapse button, a title, and menu buttons to perform common actions. Table 2 lists the menu buttons that are available in the Title area.

Table 2. Menu Buttons

Button	Name	Description
	Expand/Collapse	Expands and collapses the content control. When the content control is collapsed, a high-level summary of system monitoring data appears.
Net	Refresh icon	Indicates when information in the content control is being refreshed. When refresh is finished, this icon disappears.
**	Tools	Displays the tools menu for the content control. This button is not available on every content control, only when there are additional actions associated with the content control.
3	Help	Launches context sensitive help for this content control.

Table 2. Menu Buttons (Continued)

Button	Name	Description
0	Add to favorites tab	Places a copy of the content control on the Favorites tab. This button only appears when the content control is not already on the Favorites tab.
②	Remove from favorites tab	Removes the content control from the Favorites tab. This button only appears when the content control is on the Favorites tab.

- Header: Some content controls display important high-level information that could not be displayed in the Title area. The Header area appears even when the content control is collapsed.
- **Content**: Displays the main diagnostic information for the content control. This area is hidden when the content control is collapsed.

Some content controls also provide the following features:

Gripper: Depending on the type of data in the content control, some content controls allow
you to customize the height or width of the control. These controls have a gripper in the
bottom-right corner as shown in Figure 6.


Figure 6. A Content Control with a Gripper




• **Data Grid Filtering**: You can filter columns in the data grids. Columns that can be filtered are indicated with a filter () icon.

To filter a column:


a. Click (Filter column) in a column.

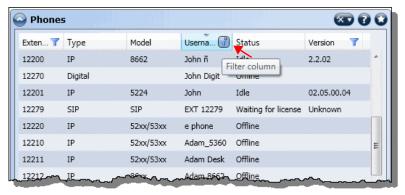

This puts the column into filter mode and displays a text box as shown below.

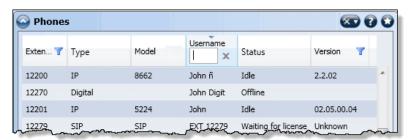

b. Type characters you want to filter in the text box. As you type characters, possible matches are filtered in the column.

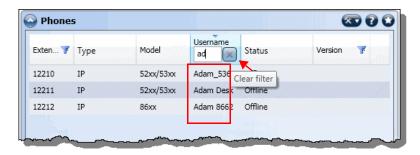


To cancel filtering:

Click (Clear filter). The column is taken out of filter mode.

System Connection Section

Figure 7 shows an example of the System Connection section.

Figure 7. System Connection Section

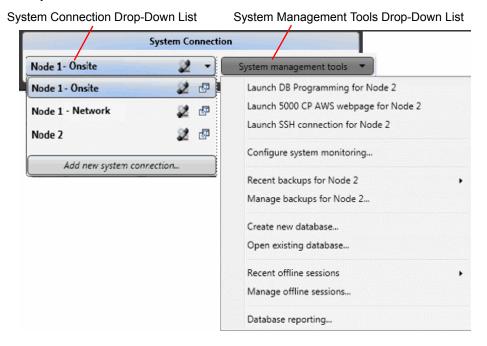

The System Connection section has the following drop-down lists that contain buttons and options for programing system connections:

- System Connection
- System Management Tools

System Connection

The System Connection drop-down list displays a list of the programmed system connections. You can edit or delete connections individually, or manage and view the backups for a connection. The box also includes menus for adding a new system and managing system connections.

The buttons that are provided in the list are:


- [Open in new window): Opens the System Administration & Diagnostics application in new window.

System Connection Network Groups

With v5.0 or later, the System Connections drop-down list displays system connections by network group. When a system connection is part of a network group, it is displayed within the network group section. The network group list can be expanded or collapsed.

All ungrouped system connections are displayed below the grouped connections in a section titled "Not Networked." If none of the system connections are in network groups, the drop-down list does not display any network groups. Figure 8 on page 16 shows an example of system connection network groups.

Figure 8. System Connection Drop-Down List

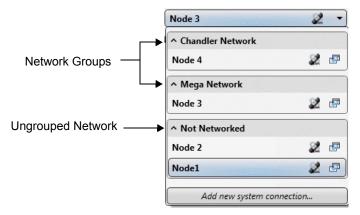

Using the System Connections drop-down list, you can add/remove connections from a network group. You can also bring up the Manage network groups window. For details, refer to the *Mitel System Administration & Diagnostics Help*.

System Management Tools

The System Management Tools drop-down list provides access to the following tools:

- DB Programming
- 5000 CP Administrative Web Session (AWS)
- Secure Shell (SSH) connection (PuTTY)


From this menu, you can also configure system monitoring (for Mitel Support users only), launch or manage database backups, create new databases, open existing databases, resume or manage a previously saved offline DB Programming sessions, and view database reporting.

System Monitoring Section

The System Monitoring section contains the buttons to start, pause, stop, and refresh diagnostic updates, alarm counts, system monitoring status information, and a button to expand/collapse the system monitoring content area.

Figure 9 shows the System Monitoring section.

Figure 9. System Monitoring Section



Buttons

Table 3 shows buttons for managing diagnostic updates.

Table 3. System Monitoring Buttons

Button (Name)	Description
▶ (Start monitoring system)	Starts or resumes diagnostic updates.
II (Pause data updates)	Pauses diagnostic updates.
■ (Stop monitoring system)	Stops diagnostic updates.
	Refreshes diagnostic update.

Alarm Counts

The alarm counts area contains high-level system information. This includes the number of critical, major, and minor alarms.

This area also displays the overall system status. Statuses include Unknown, Good, Moderate, and Fair. For the Moderate and Fair statuses, an information icon is displayed next to the status with a tooltip that provides more information.

To view the filtered list of alarms:

Click one of the counts. This opens a new window that shows the filtered list of alarms.

Menu Buttons

Table 2 lists the available menu buttons (see 7 in Figure 2 on page 8) and their brief descriptions. For detailed information, see the appropriate pages.

Table 4. Menu Buttons

Button	Name	Description			
₹ ▼	Utility	(Applicable to Mitel Support users only.)			
		Launches the following utilities:			
		5000 CP Database Converter: Converts an older database to newer version.			
		 5000 CP MOH (Music-on-Hold) Converter: Converts audio files to the proper format (.n64u) for the MOH feature. 			
		5000 CP Test and Repair: Tests databases for corruption.			
		 Upload Utility: Uploads different versions of software to cards, trunks, or IP devices. 			
3	Setup	Accesses the following configuration areas:			
		 Options: Configures various system-wide options, advanced settings, and global settings for Scheduled Backup. 			
		Manage system connections: Presents a list of programmed connections, and then you can add, edit, or delete a connection.			
		Export settings: Exports System Administration & Diagnostics settings to a file.			
		 Import settings: Imports settings previously exported from the System Administration & Diagnostics application or from any v3.2 and prior version of Session Manager. 			
?~	Help	Accesses the following items:			
		Help: Launches the context sensitive System Administration & Diagnostics Help.			
		System alarms help: Launches the System Alarms Help window that lists all system alarms and allows you to view the help for any alarm.			
		Tutorial: Launches the System Administration & Diagnostics User Tutorial.			
		About: Launches a window that displays System Administration & Diagnostics version, copyright information, a link to the company Web site, and the company logo.			

Expand/Collapse Button

You can expand or collapse the lower content area using the expand/collapse button. The expanded or collapsed state of the window as well as the window location and expanded size are saved when you close the application and restored when you launch the application. See Figure 2 on page 8 for an example of the collapsed System Administration & Diagnostics

To collapse or expand the System Administration & Diagnostics window:




Tooltips

If applicable, a tooltip appears to further explain descriptions or status of the selected field or menu. Fields where tooltips are available are described throughout the guide.

To view the information in a tooltip:

Move the pointer over the area where you want to view the tooltip information. If a tooltip is available, a screen similar to the one below appears.


Figure 10. Tooltip

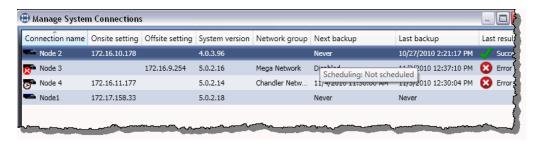

Warning Message Boxes

The System Administration & Diagnostics application may display a warning message box to bring an issue to your attention. Figure 11 shows an example of the Delete Connection warning message box.

Figure 11. Delete Connection Warning Message Box

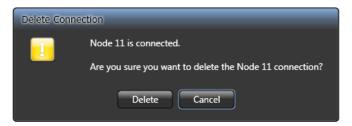

A warning message box may contain any of the following connection issues:

- Test Onsite/Offsite Connections
- Activate Connections
- Delete Connections
- Disconnect Connections
- Save Connections
- Close Application

Installing and Launching the Application

Introduction	22
Installing the Application	22
Launching the Application	24
Importing Connections	25
Adding Connections Manually	25
Exiting without Adding or Importing Connections	28
Enabling an On-Demand Remote Connection from a phone	29
Upgrading from Older Software	30
Programming the Application	31

Introduction

This chapter provides information for installing and configuring the System Administration & Diagnostics application.

Installing the Application

The following section describes the instructions for installing the System Administration & Diagnostics application. The System Administration & Diagnostics application installs the following utilities and tools automatically:

- Mitel Database Programming
- 5000 CP Administrative Web Session
- SSH connection (PuTTY)
- 5000 CP Database Converter
- 5000 CP MOH Converter
- 5000 CP Test and Repair
- Upload Utility

NOTES

System Administration & Diagnostics provides access to all DB Programming features for all DB Programming versions. If you attempt to launch Session Manger after upgrading to System Administration & Diagnostics, a notice appears indicating that you need to use System Administration & Diagnostics to manage system connections.

You must have local administrative rights to install the application.

To install System Administration & Diagnostics and DB Programming:

- Verify that Microsoft Windows is running (Windows XP, Windows Vista, or Windows 7) and that you have local administrative rights.
- Insert the System Administration & Diagnostics / DB Programming DVD into the DVD-ROM drive, or download the software from <u>Mitel Software Downloads</u> (http://portal.mitel.com/wps/myportal/MOLPageDetails?WCM_GLOBAL_CONTEXT=/wps/wcm/myconnect/mitelonline/MitelOnline/Home/Technical/Software+Downloads+%28SA%29). Note that you must first log on to <u>Mitel OnLine</u> (http://portal.mitel.com/wps/myportal/MOLHome) in order to access this site.
- Open the DVD folder (if necessary), and then double-click SAaDDBP_X_X_X_X-core_DBP_Y_Y_Y-plugin.exe, where the X_X_X_X indicates the System Administration & Diagnostics / DB Programming core version number and Y_Y_Y_Y indicates the DB Programming version number. The Mitel 5000 CP System Administration & Diagnostics and Database Programming Installation Wizard appears.
- Follow the instructions in the wizard to complete the System Administration & Diagnostics and DB Programming installations.

To install DB Programming separately from System Administration & Diagnostics:

- Verify that Microsoft Windows is running (Windows XP, Windows Vista, or Windows 7) and that you have local administrative rights.
- Insert the System Administration & Diagnostics / DB Programming DVD into the DVD-ROM drive, or download the software from <u>Mitel Software Downloads</u> (http://portal.mitel.com/wps/myportal/MOLPageDetails?WCM_GLOBAL_CONTEXT=/wps/wcm/myconnect/mitelonline/MitelOnline/Home/Technical/Software+Downloads+%28SA%29). Note that you must first log on to <u>Mitel OnLine</u> (http://portal.mitel.com/wps/myportal/MOLHome) in order to access this site.
- 3. Open the DVD folder (if necessary), and then double-click **DBP_Y_Y_Y_Y-plugin.exe**, where the Y_Y_Y_Y indicates the DB Programming version number. The Mitel 5000 CP Database Programming Installation Wizard appears.
- 4. Follow the instructions in the wizard to complete the DB Programming installation.

Launching the Application

The following section describes how to launch the System Administration & Diagnostics application.

NOTE

You must have local administrative rights to launch the application.

To launch the System Administration & Diagnostics application:

 Select Start – All Programs – Mitel System Administration & Diagnostics. If there are no programmed connections, the System Administration & Diagnostics Welcome window appears.



When System Administration & Diagnostics is installed on a computer, system connections programmed on the computer either by a previous installation of System Administration & Diagnostics or an earlier version of DB Programming are preserved. If the connections were programmed using an earlier version of DB Programming (previously known as "sessions" programmed in the Session Manager used for pre-v4.0 systems), those connections are automatically imported into the System Administration & Diagnostics application. If the installation is an upgrade from an earlier version of System Administration & Diagnostics, the system connections are simply preserved. In either of those cases, the Welcome Window is not shown.

- 2. Do one of the following:
 - Importing Connections on page 25
 - Adding Connections Manually on page 25
 - Exiting without Adding or Importing Connections on page 28

When the System Administration & Diagnostics application is connecting to a system, the Information bar displays any of the following information:

- Connecting Information
- Success Information
- System Status Information
- Warning Information
- Failure Information
- Waiting/Disconnecting/Cancelling Information
- Connection Retry Information
- · Disconnected Information

The Add/Edit System Connection dialog box also contains the Backup tab. Refer to the Enabling Scheduled Backups help topic in the *Mitel System Administration & Diagnostics Help* for details.

For additional information about the System Connection section, refer to the Managing System Connections help topic in the *Mitel System Administration & Diagnostics Help*.

Importing Connections

This section explains how to import connections.

To import connections:

- If you have connections saved in a file, exported either from System Administration & Diagnostics or from previous use of Session Manager used for pre-v4.0 systems, select Import connections. The Import File Selection dialog box appears.
- 2. Click Browse.
- 3. Select the source file, and then click **OK**.

Adding Connections Manually

This section explains how to add connections manually.

To add connections manually:

 Select Add connections manually. When the Manage System Connections window appears, select Add to add a connection. The Add System Connection dialog box appears. The red outlining of certain fields indicates those fields currently do not hold valid settings.

Tooltip: When you move the pointer over the field, the tooltip shows an explanation of the error.

NOTE

IP addresses and hostnames are not validated at the time of programming a connection, because the system might not be online at the time. These can only be validated at the time of connection.



- In the Connection name field in the Connection tab, enter the name of the connection. This name will be used:
 - in the list on the main window,
 - for DB Programming session name, and
 - in the task name for Scheduled Backups.

- In the Onsite IP address/Hostname field, type the IP address/hostname of the 5000 CP node that you are using when you are onsite (inside the LAN). It is blank by default.
- 4. Program the Offsite Connection section.
 - In the Offsite Connection field, select the method that you are using to connect when you are offsite (outside the LAN). The options are I don't connect offsite (default), Modem, Network, and Remote Configuration.
 - b. If you are using the offsite connection, do one of the following:
 - For a Modem connection: Type the number to dial to reach the 5000 CP modem (up to 128 of any characters).
 - For a Network connection: Type the IP address/hostname of a 5000 CP node when the connection is offsite.
 - For a Remote Configuration connection: This option appears only if the Remote Configuration feature is installed on the computer. To enable an ondemand remote connection, you must establish the connection in both System Administration & Diagnostics and a system phone. For complete information about Remote Configuration, refer to the *Mitel 5000 CP Features* and *Programming Guide*, part number 580.8006.

Type the following information:

- Proxy server IP address/hostname: Type the IP address or hostname of the Proxy Server. It must match the IP address or hostname programmed in DB Programming for the node. Because the IP address can change, Mitel recommends that you use the hostname. For example, if the server is moved to a new location, the IP address may change, but it will still be assigned to the original hostname.
- Proxy server IP port: Type the IP port used for connecting to the Proxy Server. The valid range is 1-65535; the default value is 1194. This field appears only when the Show IP ports option is enabled in the Advanced tab in the Options menu.
- License key ID: Type the 5000 CP node license key ID, which identifies the system (up to 14 digits or characters). To find the license ID key, dial 347 on any phone on the 5000 CP in which you are connecting. See Enabling an On-Demand Remote Connection from a phone on page 29.
- PIN: Type the PIN to be used when connecting to the 5000 node (up to 4 digits).
- Proxy server username: Type the username for logging into the Proxy Server (supplied by Customer Care personnel.).
- Proxy server password: Type the password for logging into the Proxy Server (supplied by Customer Care personnel).

System Administration & Diagnostics then registers with the Remote Proxy Server. This may take a few minutes. A progress message displays while the connection is established.

If you receive an error message indicating that the connection to the Remote Proxy Server failed because a socket error occurred, contact a Customer Care representative for assistance.

- 5. Program the System Account section.
 - In the System Account section, select Remember username and password to enable the username and password fields.
 - b. Type the user name (up to 8 characters) and password (up to 24 characters) to log on to the 5000 CP.

For v4.0 and later systems: The user name/password pair entered in the System Account field can be any user name/password pair programmed in System Accounts in DB Programming for the system to which the connection applies. By default, an administrator (admin) account exists in all databases (with <code>itpassw</code> for the password). When you are logged in as "admin" in DB Programming, you can enable a support account and create additional accounts. You can also assign limited access rights to the additional accounts, such that they may not be able to do certain types of programming or use certain features (for example, Web page and System Monitoring). Any of these system accounts can be entered in the System Account section. When the connection is established, the System Administration & Diagnostics application learns the privileges of the account being used and warns you accordingly.

For v3.2 and earlier systems: Instead of having one password for system access, there was a password for each access method. Therefore, you must program all of the passwords in the system to be the same to make use of the available functionality in System Administration & Diagnostics. This includes Message Print, SMDR, System Monitor, Web/SSH, and DB Programming. For the System Connection, enter the Web page user name and common password in the System Account section. Refer to the Launching a pre-v4.0 DB Programming help topic in the Mitel System Administration & Diagnostics Help for details about launching a pre-v4.0 DB Programming.

- 6. Program the Network Group section.
 - a. Select the This system is part of a network check box.
 - b. (Optional) To include this system connection in a network group, select an existing network group from the Network group drop-down list in the Network Group section.
 - c. (Optional) To manage network groups, click **Manage network groups** in the Network Group section. Refer to the Managing Network Groups help topic in the *Mitel System Administration & Diagnostics Help* for details.
- 7. Program the MAS Server section.
 - a. If a Mitel Applications Suite (MAS) server is installed on the system, select **The system has a MAS server**. Additional fields appear in the MAS Server area.
 - b. In the **MAS server IP address/Hostname** field, type the following information:
 - MAS server IP address/Hostname: The IP address or hostname for the MAS Server associated with the system.
 - MAS server web listening port: The listening port for the MAS Server. The range is 1-65535; the default value is 443. This field appears only when the Show IP ports option is enabled in the Advanced tab in the Options menu.

8. Program the IP Ports section (this field appears only when the Show IP ports option is enabled in the Advanced Settings menu).

In the IP Ports field, type the following information:

- Web listening port: The port number that is used every time a connection is made by System Administration & Diagnostics to a system (the connection is verified via a Web request). It is also used to access the Web page and for system monitoring on a v4.0 or later system. The range is 1-65535; the default value is 443.
- Listening port: The port number that is used by some types of system monitoring and for DB Programming. The range is 1-65535; the default value is 44000.
- SSH server port: The port number that is used for SSH connections. The range is 1-65535; the default value is 22.
- Click Test onsite connection and Test offsite connection to test the connections. The
 Test button is available only when valid programming is entered for the connection.
 Refer to the Test Onsite/Offsite Connection Warnings and Operations help topic in the
 Mitel System Administration & Diagnostics Help for details about a connection test.
- 10. Click Save connection to save the changes. This option is available only when valid programming is entered for the connection. Clicking this option takes you back to the System Connections window. Click the red X to close, then click on drop-down list to select the newly programmed connection.
- 11. If you click **Save connection** without typing a username and password, a dialog box appears prompting you to type the username and password.
 - a. Type the username and password, and then select Remember username and password if you want the application to remember the account information. If you do not select the check box, entered credentials are saved for the duration of the session, such that you will not be re-prompted for the information until exiting from the session and starting it up again, or starting up a new instance of System Administration and Diagnostics.
 - b. Click **Connect**. If there are any invalid entries, an error message appears.
- 12. If there is an active connection that exists, the Activate Connection dialog box appears prompting whether you want to activate the new connection. Click Activate or Do not activate. If both onsite and offsite connections are programmed, click Active onsite or Active offsite to pick the connection, or click Do not activate.

To exit from the connection programming without adding a connection:

- Select Cancel. The Cancel Edit dialog box appears prompting whether you want to discard the changes.
- 2. Click **Yes** to discard changes or **No** to return to the window.

Exiting without Adding or Importing Connections

This section explains how to exit without adding or importing connections.

To exit without adding or importing connections:

Click **Do not add connections**. The System Administration & Diagnostics Welcome window disappears.

Enabling an On-Demand Remote Connection from a phone

You can use any 5000 CP phone to enable or disable Remote Configuration sessions.

NOTE

Disabling Remote Configuration from a system phone prevents remote users from accessing the system in which the phone is registered.

To enable Remote Configuration from a system phone, the remote technician must provide you with the personal identification number (PIN) that is registered with the Remote Proxy Server. The remote technician must also enter the 5000 CP license key ID, or Hardware Against Software Piracy (HASP) key. If necessary, you can use any system phone to view the HASP key and provide it to the remote technician, as described below.

To enable a Remote Configuration session:

- On any system phone, dial 342. ENTER PIN appears.
- Enter the PIN number (supplied by the remote technician), and then press #. REMOTE CONFIG ENABLED appears.

To end a Remote Configuration session:

Dial 343. REMOTE CONFIG DISABLED appears.

To display the license key ID (HASP key):

Dial 347. HW SERIAL NUM < number > appears.

To reset the Remote Configuration session:

Dial 344.

Upgrading from Older Software

When System Administration & Diagnostics is installed, it looks for previously existing session settings and associated databases that are stored on the computer. System connections are automatically created from all valid online sessions found, and offline sessions are automatically created from all valid offline sessions found.

If System Administration & Diagnostics is being installed on a computer without previously stored sessions, you can import settings from another computer later, as long as they have been exported from the Session Manager (used for pre-v4.0 systems) to a file. Refer to the Programming Import Settings help topic in the *Mitel System Administration & Diagnostics Help* for details.

Databases associated with offline sessions only can be transferred to a new computer via the database save operation: using the computer on which an offline session resides, open the offline session (using the Local tab), save the database, and then copy the saved database file to the new computer. You can then use the Open existing database option to access the database. Refer to the Opening Existing Database help topic in the *Mitel System Administration & Diagnostics Help* for details.

Programming the Application

For programming instructions, refer to the Mitel System Administration & Diagnostics Help.

To access the online help:

Press **F1** or the Help menu button () in the upper-right corner of the application interface.

The Help contains the following information:

- About System Administration & Diagnostics: Provides information about an overview of the System Administration & Diagnostics application. This is the same information described in the Overview chapter in this guide.
- **Understanding the Interface**: Summarizes the functionality of the System Administration & Diagnostics UI. This is the same information described in the Understanding the Interface chapter in this guide.
- Getting Started: Provides instructions for launching the application and information for upgrading. This section also provides the instructions for programming scheduled backups.
- Managing System Connections: Provides information for programming, managing, and using system connections, DB Programming, and management tools.
- **Using System Monitoring Tools**: Provides information for programming, managing, and using system monitoring content controls and tools.
- **Using the Menu Buttons**: Provides information for programming, managing, and using the Utilities, Setup, and Help menu buttons.
- **Diagnostics and Troubleshooting**: Provides information that helps you to diagnose and troubleshoot issues that are associated with System Administration and Diagnostics.

Index

Н Α About this Guide 3 Hardware Requirements 6 Adding Connections Manually 25 Header 13 Alarm Counts 17 Application installing 22 launching 24 Importing Connections 25 programming 31 Information Bar 9 Application, installing and launching 21 Installing the Application 22 Interface, understanding 7 B Introduction 2, 8, 22 Buttons 17 C Licensing 6 Compatibility 5 M Connectioms, adding 25 Connection Types 4 Menu Buttons 18 Connections Mitel Support 4 adding 25 exiting 28 importing 25 N Content 13 Content Controls 12 Navigating 9 Navigation 9 D Navigation Area 10 Network Requirements 6 Data Grid Filtering 13 DB Programming Connections 5 0 Ε Older Software, upgrading 30 On-Demand Remote Connections, enabling 29 Enabling an On-Demand Remote Connection from a phone 29 Overview 1 Exiting without Adding or Importing Connections 28 Expand/Collapse Button 18 P G Programming the Application 31 Getting Started 21 R Gripper 13

Reporting User 4

S

Software Requirements 6
Specifications 6
System Administrator 4
System Connection 15
System Connection Header 9
System Connection Network Groups 15
System Connection Section 15
System Connections 4
System Management Tools 16
System Monitoring Section 17

Т

Title 12
Title Bar 9
Tooltips 19

U

Upgrading 30
User Types 4
Mitel support 4
reporting user 4
system administrator 4



Warning Message Boxes 19

Part No. 550.8125 Issue 5.0, February 2011



Global Headquarters	U.S.	EMEA	CALA	Asia Pacific
Tel: +1(613) 592-2122	Tel: +1(480) 961-9000	Tel: +44(0)1291-430000	Tel: +1(613) 592-2122	Tel: +61(0) 2 9023 9500
Fax: +1(613) 592-4784	Fax: +1(480) 961-1370		Fay: +1(613) 592-7825	Fax: +61(0) 2 9023 9501

www.mitel.com



For more information on our worldwide office locations, visit our website at www.mitel.com/offices

THIS DOCUMENT IS PROVIDED TO YOU FOR INFORMATIONAL PURPOSES ONLY. The information furnished in this document, believed by Mitel to be accurate as of the date of its publication, is subject to change without notice. Mitel assumes no responsibility for any errors or omissions in this document and shall have no obligation to you as a result of having made this document available to you or based upon the information it contains.

M MITEL (design) is a registered trademark of Mitel Networks Corporation. All other products and services are the registered trademarks of their respective holders.